

Griplok®
INSTRUMENTATION
TUBE FITTINGS

TECHNICAL REPORT



8250 Boyle Parkway
Twinsburg, OH 44087-2200, USA

Table 1: Contents

| Section | Description | Page |
|----------------|---|-------------|
| 1.0 | Document Introduction..... | 4 |
| 2.0 | Tests and General Conclusions..... | 4 |
| 3.0 | Validation Tests and Results..... | 5 |
| 3.1 | Initial Makeup Test..... | 5 |
| 3.2 | Hydrostatic Burst Pressure Test..... | 8 |
| 3.3 | Hydraulic Impulse Pressure Test..... | 10 |
| 3.4 | Repeated Remake Test..... | 12 |
| 3.5 | Tension Force Test..... | 14 |
| 3.6 | Vibration Stress / Endurance Test..... | 16 |
| 3.7 | Intermix Assurance Test..... | 18 |
| 3.8 | Interchange Assurance Test..... | 20 |
| 3.9 | Gas Pressure Leak Test..... | 22 |
| 3.10 | Thermal Cycle, Thermal Shock Test..... | 24 |
| 3.11 | Vacuum Test..... | 26 |
| 3.12 | Low Temperature (Cryoqenic) Helium Leak Test..... | 28 |
| 4.0 | Bibliography, Equipment, References..... | 30 |

Table 1.0, Contents

Introduction

Since its inception in 1926, SSP has exhibited an expertise in the precision machining of tight tolerance, high quality fitting components. In fact, SSP's historical reputation for product quality, service and performance is recognized across the country and around the world.

In 1986, SSP relocated to its 25-acre property in Twinsburg, Ohio Southeast of Cleveland in North America's manufacturing heartland. Within its modern 165,000 square foot manufacturing facility, SSP has developed the internal ability to control its manufacturing variables as much or more than any other fittings' manufacturer. SSP designs and produces its own specialty cutting tools to proprietary standards with a 5 axis CNC tool and cutter grinder, high speed 4 axis CNC machining centers and ultra precise EDM's to allow manufacturing to the most stringent dimensional tolerances and surface finishes. Additionally, SSP's tool making capability supports an internal hot, closed-die forging operation. SSP plans, controls and performs its own metal forging operations on all elbows, tees and crosses manufactured into SSP fittings, connectors and adapters. Indeed, SSP's production capacity is among the largest single-site facilities in the entire industry with the capability to allow one-of-a kind, "specials" machining on single spindle CNC's to high volume production on multi-spindle automatics.

Furthermore, SSP's ISO9001 Quality System Certification and Registration by DNV assures conformance to the highest levels of quality. The substantial investment of time and funds to obtain and maintain such status has paid dividends for SSP and its customers in efficiencies in process and supply.

In 1993 in response to continued customer requests for an alternative product offering in the Instrumentation marketplace; strategic plans were developed to launch a division of SSP to design, manufacture and distribute American manufactured, Instrumentation quality tube fittings as a direct alternative to the registered trademark brand of Hoke Gyrolok®. The recruitment of recognized Instrumentation industry experts occurred, and a specialized design and business unit team, SSP Instrumentation, was formed. Following an ISO 9001 design process pattern, the critical elements of design planning, including the detailed documentation of design inputs and outputs occurred for the development of **Griplok®** tube fittings. Examples of such design inputs include:

- Dimensional similarity**
- Material of construction similarity**
- Installation instruction similarity**
- Operation and performance similarity**
- Brand interchangeability and intermixability**
- Corrosion resistance similarity**
- Applicable ANSI / ASME B 31.3 requirements**

To accomplish the required design plan tasks of verification and validation, a specialized Technical Center was built within SSP. In addition to the exhaustive engineering calculations for confirmation of design conformance to industry standards and other engineering developed criteria, customized NIST traceable testing equipment was procured to allow:

- Hydrostatic Proof and Burst Pressure Testing**
- Air and/or Helium Pressure Testing**
- High Vacuum Testing**
- Cyclic Vibration Testing**
- Tensile Pull Testing**
- Hydraulic Impulse Testing**
- Thermal Cycle Testing**
- Low Temperature (Cryogenic) Testing**
- High Temperature Testing**

Additional specific testing of Griplok with Hoke Gyrolok®, Swagelok®, and Parker CPI® was undertaken to confirm design compatibility and performance similarity, as well as competitive interchangeability and intermixability.

Examples of such additional testing includes:

Dimensional Measurement Comparison
Installation Make-Up Torque Comparison

Conformance to the design engineering team's prescribed acceptance criteria allows the products' release for production and distribution to the marketplace.

Section 1: Document Introduction

This document's purpose is to report, in a published format for public review, a representative sampling of the **Griplok** tube fitting's actual performance results from the Design Plan's Validation Tests. The performance results are measured against the Design Team's Approved Acceptance Criteria, which are based on meeting or exceeding the published and / or test-based performance of equivalent products from Hoke Gyrolok. A positive testing performance of the products in the Validation Tests was required to complete the final element of the design cycle and provide for the Design Release of the **Griplok** product family.

Section 2: Tests and General Conclusions of Results

The preceding table (Table 1.0) lists the major Validation Tests that were performed, and the sections which follow describe the tests and outline specific results. All products manufactured at SSP are to approved and controlled engineering documentation, to established process and quality procedures at every stage of manufacture, with fully calibrated quality and process instrumentation, using only certified and traceable materials. Tested products were selected randomly from documented normal production runs. Before and after test samples were retained for reference. All tubing used in testing meets applicable ASTM specifications, and has approved material and chemical certifications.

All SSP tests conducted on products are with laboratory equipment and instrumentation in current calibration. Trained personnel conducted tests by following approved, written test procedures. All test results were subjected to thorough engineering review and approval before internal publication.

In every case all **Griplok** test results met or exceeded the established Design Team's Acceptance Criteria for these products. As such, they also met or exceeded equivalent major competitive product performance, as measured in test data and / or reported in publications.

Section 3.0: Validation Tests and Results

Section 3.1: Initial Makeup Test

Purpose: Test determines if the tube and fitting assembly has comparable levels of assembly torque to that of Hoke Gyrolok, and achieves proper fitting makeup.

NOTE: Instrumentation Tube Fittings, due to the variances of tubing hardness and outside / inside diameters, require a certain geometric rotation of the tubing nut for proper makeup.

Assembly torque requirements vary per application and the level of torque is a general consideration, not a specification, for proper makeup.

Equipment & Configuration: Saw, tube deburring tool, vice and torque wrench. See Figures 3.1.1 - 2, Initial Makeup



Figures 3.1.1 - 2, Initial Makeup: Torque Measurement and Fitting Assembly

Test Procedure: The fitting and tube are assembled per published standard fitting makeup instructions. Torque, in inch-pounds (or foot-pounds), vs. nut tightening rotation is recorded in $\frac{1}{4}$ turn increments.

Acceptance Criteria: Fitting is to achieve proper makeup, with average assembly torque being equal to or less than Hoke[®] Gyrolok average results, and individual results being less than the Hoke[®] Gyrolok average plus 3σ . See Example Acceptance Criteria in Table 3.1.1 below.

| Tubing / Fitting | | | Acceptance Criteria | | | | | |
|------------------|-------|-------|---------------------|------|------|------|------|-----------------|
| | | | Torque, in-lb | | | | | |
| Size | Wall | W.P. | Revolutions | | | | | Ave + 3σ |
| # | in | psig | 0.25 | 0.50 | 0.75 | 1.00 | 1.25 | 1.25 |
| 8 | 0.035 | 2,450 | 38 | 105 | 172 | 216 | 249 | 387 |
| | 0.083 | 6,250 | 37 | 111 | 280 | 385 | 493 | 781 |

Table 3.1.1, Example Initial Makeup Torque Acceptance Criteria

Test Results: Example results are shown in Table 3.1.2 below.

Results: Initial Makeup Torque Test

| Sample No. | Initial Makeup Torque, in-lb | | | | | | | | | | | | Test |
|------------|------------------------------|------|------|-------|-------------|-----------|-------------|------|------|-------|-------------|-----------|---------------|
| | Size # | 8 | x | 0.035 | Wall Tubing | | Size # | 8 | x | 0.083 | Wall Tubing | | |
| | Revolutions | | | | | Pass Fail | Revolutions | | | | | Pass Fail | |
| | 0.25 | 0.50 | 0.75 | 1.00 | 1.25 | P / F | 0.25 | 0.50 | 0.75 | 1.00 | 1.25 | P / F | |
| 1 | 25 | 70 | 100 | 140 | 155 | P | 30 | 125 | 200 | 250 | 340 | P | Bite |
| 2 | 30 | 70 | 125 | 150 | 165 | P | 30 | 105 | 170 | 230 | 325 | P | |
| 3 | 40 | 70 | 90 | 125 | 130 | P | 25 | 110 | 190 | 240 | 355 | P | |
| 4 | 50 | 90 | 150 | 175 | 195 | P | 30 | 130 | 200 | 270 | 360 | P | |
| 1 | 40 | 95 | 135 | 180 | 190 | P | 30 | 120 | 245 | 340 | 450 | P | Tension |
| 2 | 40 | 70 | 100 | 155 | 170 | P | 30 | 105 | 240 | 325 | 415 | P | |
| 3 | 40 | 70 | 120 | 155 | 160 | P | 30 | 110 | 200 | 245 | 310 | P | |
| 4 | 30 | 65 | 100 | 150 | 170 | P | 30 | 125 | 190 | 290 | 415 | P | |
| 5 | 30 | 75 | 150 | 200 | 220 | P | 30 | 120 | 190 | 300 | 410 | P | |
| 1 | 30 | 75 | 135 | 160 | 175 | P | 50 | 140 | 205 | 250 | 330 | P | Gas Leak |
| 2 | 25 | 85 | 140 | 175 | 200 | P | 50 | 110 | 180 | 220 | 270 | P | |
| 3 | 30 | 90 | 115 | 160 | 180 | P | 55 | 125 | 220 | 275 | 365 | P | |
| 4 | 25 | 75 | 115 | 170 | 190 | P | 40 | 120 | 185 | 230 | 290 | P | |
| 5 | 35 | 90 | 125 | 155 | 175 | P | 45 | 145 | 210 | 300 | 385 | P | |
| 6 | 50 | 70 | 85 | 120 | 145 | P | 50 | 120 | 190 | 210 | 290 | P | |
| 7 | 45 | 80 | 115 | 170 | 185 | P | 30 | 100 | 150 | 210 | 255 | P | |
| 8 | 25 | 60 | 90 | 120 | 175 | P | 30 | 100 | 180 | 220 | 275 | P | |
| 9 | 30 | 65 | 85 | 110 | 140 | P | 40 | 110 | 195 | 230 | 295 | P | |
| 10 | 35 | 65 | 90 | 125 | 130 | P | 45 | 110 | 170 | 210 | 270 | P | |
| 11 | 30 | 70 | 90 | 110 | 165 | P | 30 | 100 | 180 | 220 | 280 | P | |
| 12 | 40 | 90 | 125 | 160 | 180 | P | 55 | 165 | 260 | 330 | 390 | P | |
| 1 | 30 | 75 | 105 | 115 | 155 | P | 60 | 110 | 210 | 2454 | 330 | P | Thermal Cycle |
| 2 | 35 | 80 | 110 | 160 | 225 | P | 70 | 145 | 200 | 230 | 335 | P | |
| 3 | 30 | 95 | 160 | 200 | 205 | P | 55 | 125 | 210 | 240 | 365 | P | |
| 4 | 30 | 75 | 110 | 125 | 155 | P | 25 | 145 | 210 | 280 | 395 | P | |
| 5 | 30 | 65 | 105 | 150 | 190 | P | 40 | 110 | 150 | 195 | 295 | P | |
| 1 | 35 | 90 | 125 | 160 | 190 | P | 40 | 120 | 205 | 310 | 400 | P | Remake |
| 2 | 25 | 70 | 100 | 125 | 145 | P | 40 | 110 | 140 | 220 | 280 | P | |
| 3 | 25 | 50 | 95 | 130 | 165 | P | 40 | 110 | 170 | 230 | 360 | P | |
| 4 | 20 | 70 | 120 | 150 | 195 | P | 30 | 125 | 220 | 285 | 350 | P | |
| 5 | 30 | 75 | 110 | 135 | 160 | P | 50 | 115 | 160 | 205 | 285 | P | |
| 6 | 25 | 60 | 100 | 150 | 160 | P | 30 | 105 | 165 | 225 | 295 | P | |

Table 3.1.2, Example Initial Makeup Torque Results

Conclusions: All Griplik assemblies met or exceeded the approved Acceptance Criteria.

Section 3.2: Hydrostatic Burst Pressure Test

Purpose: Test determines if the tube fitting assembly has adequate pressure-retaining capability, based on the ANSI / ASME B 31.3 maximum allowable working pressure of the tubing.

Equipment & Configuration: Two fittings are tested at a time – one on each end of a 4 ½” long piece of tubing, per Initial Makeup Test (see Section 3). Samples of both minimum and maximum recommended wall tubing (worst case conditions) are used for each tested product configuration. See Figures 3.2.1 – 3.

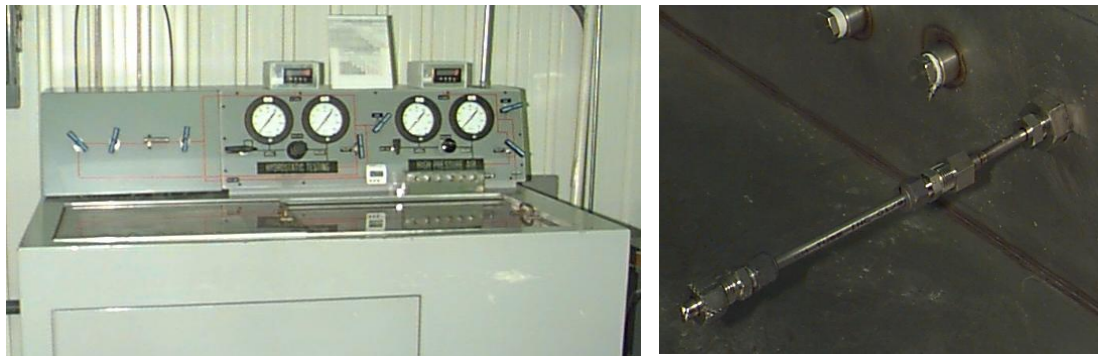


Figure 3.2.1 - 2, Burst Test Configuration



Figure 3.2.3, Burst Test Specimen

Test Procedure: The tube fitting assembly is hydrostatically pressurized in regular pressure increments which increase until tube burst is attained. The digitally displayed maximum pressure, in PSIG, - at which the tubing bursts or tubing pushes out of the fitting - is recorded.

Acceptance Criteria: The tube fitting assembly is to sustain a hydrostatic pressure, without observed leakage, exceeding a minimum of 4 times the ANSI / ASME maximum allowable working pressure of the tubing. Failure is to be by tubing burst, not by tube push out from fitting.

Test Results: Example results are shown in Table 3.2.0 below.

Results: Burst Test (Sample - Tube ends: A, B)

| Test | Sample No. | | Tubing / Fitting | | Acceptance Criteria | | Burst Test | | |
|-----------|------------|----|------------------|-------|---------------------|------------------|--------------|-----------|-----------|
| | A | B | Size | Wall | W.P. | Burst = 4 x W.P. | Actual Burst | Fail Type | Pass Fail |
| | # | # | # | in | psig | psig | psig | n/a | P / F |
| Impulse | 1 | 2 | 8 | 0.035 | 2,450 | 9,800 | 12,290 | Tube | P |
| | 3 | 4 | | | | | 12,230 | Tube | P |
| | 5 | 6 | | | | | 12,240 | Tube | P |
| | 7 | 8 | | | | | 12,300 | Tube | P |
| | 9 | 10 | | | | | 10,350 | Tube | P |
| | 11 | 12 | | | | | 10,400 | Tube | P |
| | 1 | 2 | | 0.083 | 6,250 | 25,000 | 27,940 | Tube | P |
| | 3 | 4 | | | | | 27,970 | Tube | P |
| | 5 | 6 | | | | | 27,690 | Tube | P |
| | 7 | 8 | | | | | 28,080 | Tube | P |
| | 9 | 10 | | | | | 28,100 | Tube | P |
| | 11 | 12 | | | | | 27,940 | Tube | P |
| Remake | 1 | 2 | 8 | 0.035 | 2,450 | 9,800 | 10,350 | Tube | P |
| | 3 | 4 | | | | | 12,330 | Tube | P |
| | 5 | 6 | | | | | 12,260 | Tube | P |
| | 1 | 2 | | 0.083 | 6,250 | 25,000 | 27,940 | Tube | P |
| | 3 | 4 | | | | | 28,270 | Tube | P |
| | 5 | 6 | | | | | 28,050 | Tube | P |
| Vibration | 1 | | 8 | 0.035 | 2,450 | 9,800 | 12,190 | Tube | P |
| | 2 | | | | | | 12,340 | Tube | P |
| | 3 | | | | | | 12,190 | Tube | P |
| | 4 | | | | | | 12,190 | Tube | P |

Table 3.2.0, Example Burst Test Results

Conclusions: All Griplik assemblies met or exceeded the approved Acceptance Criteria. All Griplik tube fittings sustained the required maximum allowable working pressure without leakage, and held leak free to tubing burst, without exhibiting tube push out from the fitting.

Section 3.3: Hydraulic Impulse Test

Purpose: Test determines if the tube fitting assembly can sustain extended pressure cycling without leakage.

Equipment & Configuration: For each stand manifold position, two fittings are tested at a time – one on each end of a test tube piece. Samples of both minimum and maximum recommended wall tubing (worst case conditions) are used for each tested product configuration. See Figures 3.3.1 – 2.



Figure 3.3.1 - 2, Hydraulic Impulse Test Stand and Fixture

Test Procedure: The tube fitting assembly is pressurized with hydraulic test oil in a manifold with up to 24 fittings. The hydraulic fluid temperature and the pressure cycle envelope conform to MIL-H-24135 test specification. Peak test pressure is 5,250 PSIG, sustained at 30 cycles/minute. Test oil temperature is maintained between 120°F-125°F. Following the Hydraulic Impulse Test, samples are also subjected to Burst Test.

Acceptance Criteria:

Hydraulic Impulse Test: The tube fitting assembly is to sustain pressure cycling without observed leakage for 150,000 test cycles.

Burst Test: The tube fitting assembly is to sustain a hydrostatic pressure, without observed leakage, exceeding a minimum of 4 times the ANSI / ASME maximum allowable working pressure of the tubing. Failure is to be by tubing burst, not by tube push out from fitting.

Test Results: Example results are shown in Table 3.3.0 below

Results: Impulse Test, followed by Burst Test:

| Test | Sample No. | | Tubing / Fitting | | Acceptance Criteria | | | Impulse Test | | |
|---------|------------|----|------------------|-------|---------------------|-------------|-------------|--------------------------|-------------|-----------|
| | A | B | Size | Wall | Impulse Cycles | Test Press. | Leak | Cycles without Failure | Leak | Pass Fail |
| | # | # | # | in | cycles | psig | Leak / None | cycles x 10 ³ | Leak / None | P / F |
| Impulse | 1 | 2 | 8 | 0.035 | 150,000 | 5,250 | None | 150 | None | P |
| | 3 | 4 | | | | | | 150 | None | P |
| | 5 | 6 | | | | | | 150 | None | P |
| | 7 | 8 | | | | | | 150 | None | P |
| | 9 | 10 | | | | | | 150 | None | P |
| | 11 | 12 | | | | | | 150 | None | P |
| | 1 | 2 | | 0.083 | 150,000 | 5,250 | None | 150 | None | P |
| | 3 | 4 | | | | | | 150 | None | P |
| | 5 | 6 | | | | | | 150 | None | P |
| | 7 | 8 | | | | | | 150 | None | P |
| | 9 | 10 | | | | | | 150 | None | P |
| | 11 | 12 | | | | | | 150 | None | P |

| Test | Sample No. | | Tubing / Fitting | | Acceptance Criteria | | Burst Test | | |
|---------|------------|----|------------------|-------|---------------------|------------------|--------------|-----------|-----------|
| | A | B | Size | Wall | W.P. | Burst = 4 x W.P. | Burst Actual | Fail Type | Pass Fail |
| | # | # | # | in | psig | psig | psig | n/a | P / F |
| Impulse | 1 | 2 | 8 | 0.035 | 2,450 | 9,800 | 12,290 | burst | P |
| | 3 | 4 | | | | | 12,230 | burst | P |
| | 5 | 6 | | | | | 12,240 | burst | P |
| | 7 | 8 | | | | | 12,300 | burst | P |
| | 9 | 10 | | | | | 10,350 | burst | P |
| | 11 | 12 | | | | | 10,400 | burst | P |
| | 1 | 2 | | 0.065 | 6,250 | 25,000 | 27,940 | burst | P |
| | 3 | 4 | | | | | 27,970 | burst | P |
| | 5 | 6 | | | | | 27,690 | burst | P |
| | 7 | 8 | | | | | 28,080 | burst | P |
| | 9 | 10 | | | | | 28,100 | burst | P |
| | 11 | 12 | | | | | 27,940 | leak | P |

NOTE: A.C. = Acceptance Criteria

Table 3.3.0, Example Hydraulic Impulse and Burst Test Results

Conclusions: All Griplik assemblies met or exceeded the approved Acceptance Criteria. No leakage or rupture of a Griplik tube fitting assembly was observed beneath 4X working pressure.

Section 3.4: Repeated Remake Test

Purpose: Test determines capability of the tube fitting assembly to successfully seal after repeated assembly and disassembly of a made-up tube assembly with a mating fitting. This test simulates the normal use condition where fittings are repeatedly disassembled from fittings for fluid system service or maintenance, and reassembled with additional tightening.

Equipment & Configuration: Two fittings are tested at a time – one on each end of a 4 ½” long piece of tube, per Initial Makeup Test (see Section 3). Samples of both minimum and maximum recommended wall tubing (worst case conditions) are used for each tested product configuration. See Figure 3.4.1, Repeated Remake Test



Figure 3.4.1, Repeated Remake Test (Size 8 Griplik)

Test Procedure: To simulate repeated remake conditions, the tube fitting is disassembled and assembled (tightening from the preceding installation position an additional 1/12 turn – or 30° each time) at each reassembly, for five successive times. This is followed by air pressure testing to the maximum recommended working pressure of the tubing, under water to observe leakage. After each disassembly of the tube fitting assembly it is examined for absence of the following Remake Failure Criteria:

Tube Sticking, Body Swelling, Nut Sticking, Thread Galling, Ferrule Set, Ferrule Galling, Body Denting, Excessive Torque, Tube push out or burst.

Acceptance Criteria: The tube fitting assembly is to sustain an air booster test pressure, PSIG, of the ANSI / ASME maximum allowable working pressure of the tubing, up to a maximum pressure of 10,000 PSIG. Failure is either any observed air leakage bubble, or the presence of any of the above Remake Failure Criteria.

Test Results: Example results are shown in Table 3.4.0 below.

| Gas Leak Test | | | | | |
|-----------------------------|---------------|----------------|------------------|----------------|------------------|
| Tubing Size #: | | | | | 8 |
| Tubing Wall: | | 0.035 | in | 0.083 | in |
| Gas Leak Test | | 2,450 | psig | 6,250 | psig |
| Acceptance Criteria: | | No Leak | Leak / None | No Leak | Leak / None |
| Sample | Remake | Leak | Pass Fail | Leak | Pass Fail |
| # | # | Leak / None | P / F | Leak / None | P / F |
| 1 | 1 | None | P | None | P |
| | 2 | None | P | None | P |
| | 3 | None | P | None | P |
| | 4 | None | P | None | P |
| | 5 | None | P | None | P |
| 2 | 1 | None | P | None | P |
| | 2 | None | P | None | P |
| | 3 | None | P | None | P |
| | 4 | None | P | None | P |
| | 5 | None | P | None | P |
| 3 | 1 | None | P | None | P |
| | 2 | None | P | None | P |
| | 3 | None | P | None | P |
| | 4 | None | P | None | P |
| | 5 | None | P | None | P |
| 4 | 1 | None | P | None | P |
| | 2 | None | P | None | P |
| | 3 | None | P | None | P |
| | 4 | None | P | None | P |
| | 5 | None | P | None | P |
| 5 | 1 | None | P | None | P |
| | 2 | None | P | None | P |
| | 3 | None | P | None | P |
| | 4 | None | P | None | P |
| | 5 | None | P | None | P |
| 6 | 1 | None | P | None | P |
| | 2 | None | P | None | P |
| | 3 | None | P | None | P |
| | 4 | None | P | None | P |
| | 5 | None | P | None | P |

Table 3.4.0, Example Repeated Remake Test Results

Conclusions: All Griplik assemblies met or exceeded the approved Acceptance Criteria. No leakage or Remake failures were observed in any Griplik tube fitting assemblies.

Section 3.5: Tension Test

Purpose: Test determines if the tube fitting assembly has the capability to sustain axial forces equivalent to the hydrostatic end force caused by approaching four times tubing working pressure. This test simulates end loading of straight, stiff, tube assemblies subjected to large end loads, as occur with structural deflection and thermal expansions.

Equipment & Configuration: One fitting is assembled on the end of a test tube, per Initial Makeup Test (see Section 3). Tensile loads are applied via a Tensile Test machine. Samples of both minimum and maximum recommended wall tubing (worst case conditions) are used for each tested product configuration. See Figure 3.5.1.

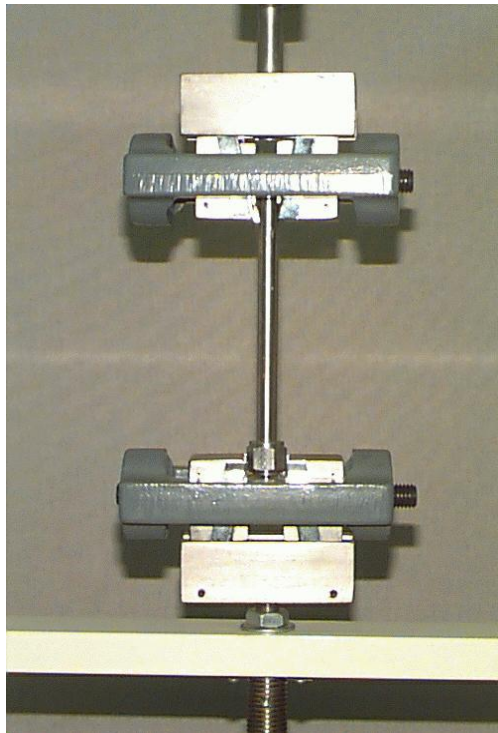


Figure 3.5.1, Tension Test Configuration.

Test Procedure: The tube fitting assembly is axially loaded in tension, and increasing loads are applied until tubing pull out is observed. The maximum load sustained by the fitting, in pounds, is recorded by digital force instrumentation.

Acceptance Criteria: The tube fitting assembly is to sustain an end force approaching that equivalent to the end force produced by 4 times the ANSI / ASME maximum allowable working pressure of the tubing. Failure is a pull out force less than this equivalent end load.

Test Results: Example results are shown in Table 3.5.0 below.

Results: Tension Test

| Sample No. | Tubing / Fitting | | Acceptance Criteria | | Tension Test | | | | |
|------------|------------------|-------|---------------------|---|--------------|-----------------------------------|----------------------|-----------|-----------|
| | Size | Wall | W.P. | Burst = 4 x W.P. (basis of Pullout Force) | Tubing O.D. | Pullout Force (based on 4 x W.P.) | Actual Pullout Force | Fail Type | Pass Fail |
| # | # | in | psig | psig | in | lb | lb | # | P / F |
| 1 | 8 | 0.028 | 2,450 | 9,800 | 0.5000 | 1,924 | 2,734 | 1 | P |
| 2 | | | | | 0.5000 | 1,924 | 2,622 | 1 | P |
| 3 | | | | | 0.5000 | 1,924 | 2,790 | 1 | P |
| 4 | | | | | 0.5000 | 1,924 | 2,808 | 1 | P |
| 5 | | | | | 0.5000 | 1,924 | 2,780 | 1 | P |
| 1 | | 0.083 | 6,250 | 25,000 | 0.4990 | 4,889 | 5,694 | 1 | P |
| 2 | | | | | 0.4990 | 4,889 | 5,960 | 1 | P |
| 3 | | | | | 0.4990 | 4,889 | 5,938 | 1 | P |
| 4 | | | | | 0.4990 | 4,889 | 5,780 | 1 | P |
| 5 | | | | | 0.4990 | 4,889 | 5,660 | 1 | P |

NOTE: A.C. = Acceptance Criteria

FAIL TYPE #:

- *1 Pullout
- *2 Broke in Tension at the rear ferrule.
- *3 Tube broke in Tension at mid-length.

Table 3.5.0, Example Tension Test Results

Conclusions: All Griplik assemblies met or exceeded the approved Acceptance Criteria. Observed pull out forces generally exceeded the equivalent of four times tubing working pressure for all Griplik tube fitting assemblies.

Section 3.6: Vibration Test

Purpose: Test determines if the tube fitting assembly has high resistance to vibration based fatigue when simultaneously exposed to 1.6 times tubing maximum allowable working pressure, based on the ANSI / ASME B 31.3 maximum allowable working pressure of the tubing.

Equipment & Configuration: One fitting is tested at a time in each station of the stand. The fitting is assembled to one end of a test tube, made up per Initial Makeup Test (see Section 3). A small format strain gage is mounted axially on the tube next to the fitting nut, and the gage is read by peak stress detecting strain gage instrumentation. A motor coaxial to the fitting axis turns a faceplate containing a spherical bearing that is radially offset to produce cyclic strain on the tested tube fitting assembly.

Samples of tubing with the minimum recommended wall (worst case condition) are used for each tested product configuration. See Figures 3.6.1 - 2.

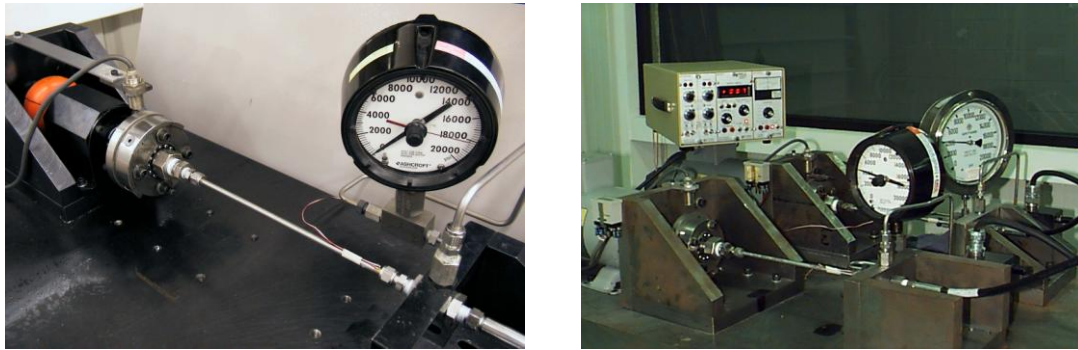


Figure 3.6.1 - 2, Vibration Test Stand and Test Configuration

Test Procedure: The motor faceplate is adjusted to produce a maximum stress adjacent the tube fitting nut equal to 60% of the tubing yield stress (YS), in KSI, as digitally indicated on the strain gage instrumentation. The tube fitting assembly is hydrostatically pressurized to 1.6 times the tubing maximum allowable working pressure and isolated from the pump by a valve. A digital counter counts revolutions of the motor faceplate (equal to the number of complete stress cycles from maximum tensile to maximum compressive stress of 60% of YS). A pressure switch stops the test on any loss of pressure during the test.

Acceptance Criteria: The tube fitting assembly is to sustain a combination of hydrostatic pressure equal to 1.6 times the ANSI / ASME maximum allowable working pressure of the tubing, and 10 million stress cycles. Failure is any loss of pressure in the tube fitting assembly.

Test Results: Example results are shown in Table 3.6.0 below.

Configuration: Vibration Test

| Strain gage data: | | |
|--------------------------|-------------------|------|
| Item | Value | Unit |
| Lot number: | R-A63BD06 | n/a |
| Stock number: | EA-06-062EN-350 | n/a |
| Gage factor: | 2.08±0.5% @ 24° C | dmls |
| Gage Excitation Voltage: | 5 | V |
| Peak Stress value: | 12,000 | psi |
| Modulus of Elasticity: | 30,000,000 | psi |
| Strain setting: | 400 | με |

Results: Vibration Test

| Test | Sample No. | Tubing / Fitting | | Acceptance Criteria | | | Vibration Test | | |
|------------------|------------|------------------|-------|---------------------|-------------|-------------|--------------------------|-------------|-----------|
| | | Size | Wall | Vibr. Cycles | Test Press. | Leak | Cycles without Failure | Leak | Pass Fail |
| | # | # | in | cycles | psig | Leak / None | cycles x 10 ⁶ | Leak / None | P / F |
| <i>Vibration</i> | 1 | 8 | 0.035 | 10,000,000 | 3,920 | None | 10 | None | P |
| | 2 | | | | | | 10 | None | P |
| | 3 | | | | | | 10 | None | P |
| | 4 | | | | | | 10 | None | P |

Results: Burst Test after Vibration Test

| Test | Sample No. | Tubing | | | | Burst Test | | |
|------------------|------------|--------|-------|-------|-----------------------|--------------|-----------|-----------|
| | | Size | Wall | W.P. | Burst A.C. = 4 x W.P. | Actual Burst | Fail Type | Pass Fail |
| | # | # | in | psig | psig | psig | n/a | P / F |
| <i>Vibration</i> | 1 | 8 | 0.035 | 2,450 | 9,800 | 12,190 | Tube | P |
| | 2 | | | | | 12,340 | Tube | P |
| | 3 | | | | | 12,190 | Tube | P |
| | 4 | | | | | 12,190 | Tube | P |

NOTE: A.C. = Acceptance Criteria

Table 3.6.0, Example Vibration Test Results

Conclusions: All Griplik assemblies met or exceeded the approved Acceptance Criteria. No observed leaks or loss of pressure occurred in any Griplik tube fitting assemblies.

Section 3.7: Intermix Test

Purpose: Test determines if all combinations of tube fitting components (nut, back ferrule, front ferrule and fitting body) of Grielok and Hoke Gyrolok can be intermixed in a tube fitting assembly. The resulting assembly must have both adequate gas and liquid pressure-retaining capability, based on ANSI / ASME B 31.3 maximum allowable working pressure of the tubing.

This test simulates the random intermixing of inventoried Grielok and Hoke Gyrolok fitting components in the field to make up tube fitting assemblies.

Equipment & Configuration: Two fittings of a given combination of fitting components are tested at a time – one on each end of a 4 ½” long piece of tube, per Initial Makeup Test (see Section 3). Samples with maximum recommended wall tubing (worst case condition) are used for each tested product configuration. See Figure 3.7.1, and Table 3.7.1.



Figure 3.7.1, Intermix Test Configuration.

| Components | Combination | | | | | | |
|---------------|-------------|---------|---------|---------|---------|---------|---------|
| | 1 | 2 | 3 | 4 | 5 | 6 | 7 |
| Body | Gyrolok | Gyrolok | Gyrolok | Grielok | Gyrolok | Grielok | Gyrolok |
| Front Ferrule | Gyrolok | Gyrolok | Grielok | Gyrolok | Gyrolok | Grielok | Grielok |
| Back Ferrule | Gyrolok | Grielok | Gyrolok | Gyrolok | Grielok | Gyrolok | Grielok |
| Nut | Grielok | Gyrolok | Gyrolok | Gyrolok | Grielok | Gyrolok | Grielok |

| Components | Combination | | | | | | |
|---------------|-------------|---------|---------|---------|---------|---------|---------|
| | 8 | 9 | 10 | 11 | 12 | 13 | 14 |
| Body | Grielok | Grielok | Grielok | Gyrolok | Grielok | Gyrolok | Grielok |
| Front Ferrule | Grielok | Grielok | Gyrolok | Grielok | Gyrolok | Grielok | Gyrolok |
| Back Ferrule | Grielok | Gyrolok | Grielok | Grielok | Gyrolok | Gyrolok | Grielok |
| Nut | Gyrolok | Grielok | Grielok | Gyrolok | Grielok | Grielok | Gyrolok |

Table 3.7.1: Intermix Test Combinations

Test Procedure: The tube fitting assembly is subjected to the Gas Leak Test (see Section 3.9), and then the Burst Test (see Section 3.2).

Acceptance Criteria: Gas Leak Test: The tube fitting assembly is to sustain an air booster test pressure, PSIG, of the ANSI / ASME maximum allowable working pressure of the tubing, up to a maximum pressure of 10,000 PSIG. Failure is any observed air leakage bubble.

Burst Test: The tube fitting assembly is to sustain a hydrostatic pressure, without observed leakage, exceeding a minimum of 4 times the ANSI / ASME maximum allowable working pressure of the tubing. Failure is to be by tubing burst, not by tube push out from fitting.

Test Results: Example results are shown in Table 3.7.2 below.

| Sample | Tubing / Fitting | | Acceptance Criteria | | | | Combination | Gas Leak Test | | Burst Test | | |
|--------|------------------|-------|---------------------|------------------|-----------------|-------------|-------------|---------------|-----------|--------------|-----------|-----------|
| | Size No. | Wall | W.P. | Burst = 4 X W.P. | Gas Leak Press. | Leak | | Leak | Pass Fail | Actual Burst | Fail Type | Pass Fail |
| # | # | in | psig | psig | psig | Leak / None | # | Leak / None | P / F | psig | n/a | P / F |
| 1 | 8 | 0.083 | 6,250 | 25,000 | 6,250 | None | 1 | None | P | 27,640 | Tube | P |
| 2 | | | | | | | | None | P | | | |
| 3 | | | | | | | 2 | None | P | 27,460 | Tube | P |
| 4 | | | | | | | | None | P | | | |
| 5 | | | | | | | 3 | None | P | 27,860 | Tube | P |
| 6 | | | | | | | | None | P | | | |
| 7 | | | | | | | 4 | None | P | 27,970 | Tube | P |
| 8 | | | | | | | | None | P | | | |
| 9 | | | | | | | 5 | None | P | 28,030 | Tube | P |
| 10 | | | | | | | | None | P | | | |
| 11 | | | | | | | 6 | None | P | 28,180 | Tube | P |
| 12 | | | | | | | | None | P | | | |
| 13 | | | | | | | 7 | None | P | 27,910 | Tube | P |
| 14 | | | | | | | | None | P | | | |
| 15 | | | | | | | 8 | None | P | 27,840 | Tube | P |
| 16 | | | | | | | | None | P | | | |
| 17 | | | | | | | 9 | None | P | 27,460 | Tube | P |
| 18 | | | | | | | | None | P | | | |
| 19 | | | | | | | 10 | None | P | 27,770 | Tube | P |
| 20 | | | | | | | | None | P | | | |
| 21 | | | | | | | 11 | None | P | 28,510 | Tube | P |
| 22 | | | | | | | | None | P | | | |
| 23 | | | | | | | 12 | None | P | 28,310 | Tube | P |
| 24 | | | | | | | | None | P | | | |
| 25 | | | | | | | 13 | None | P | 28,050 | Tube | P |
| 26 | | | | | | | | None | P | | | |
| 27 | | | | | | | 14 | None | P | 28,180 | Tube | P |
| 28 | | | | | | | | None | P | | | |

Table 3.7.2, Example Intermix Test Results

Conclusions: All Griplik assemblies met or exceeded the approved Acceptance Criteria. All Griplik tube fittings sustained the required maximum allowable working pressure without leakage, and held leak free to tubing burst without exhibiting tube push out from the fitting.

Section 3.8: Interchange Test

Purpose: Test determines if all combinations of both a tube fitting body and a tubing assembly (tube, nut, back ferrule, and front ferrule, assembled together per standard assembly instructions) of Grielok and a competitive fitting brand can be Interchanged in a complete tube fitting assembly. The resulting assembly must have both adequate gas and liquid pressure-retaining capability, based on ANSI / ASME B 31.3 maximum allowable working pressure of the tubing.

This test simulates the interchange of fitting bodies with already made up tube assemblies in the field, for components from Grielok, Swagelok, Parker CPI or Hoke Gyrolok fittings.

Equipment & Configuration: Two fittings of a given combination of fitting components are tested at a time – one on each end of a 4 ½” long test tube, per Initial Makeup Test (see Section 3). Samples with maximum recommended wall tubing (worst case condition) are used for each tested product configuration. See Figures 3.8.1 – 2.

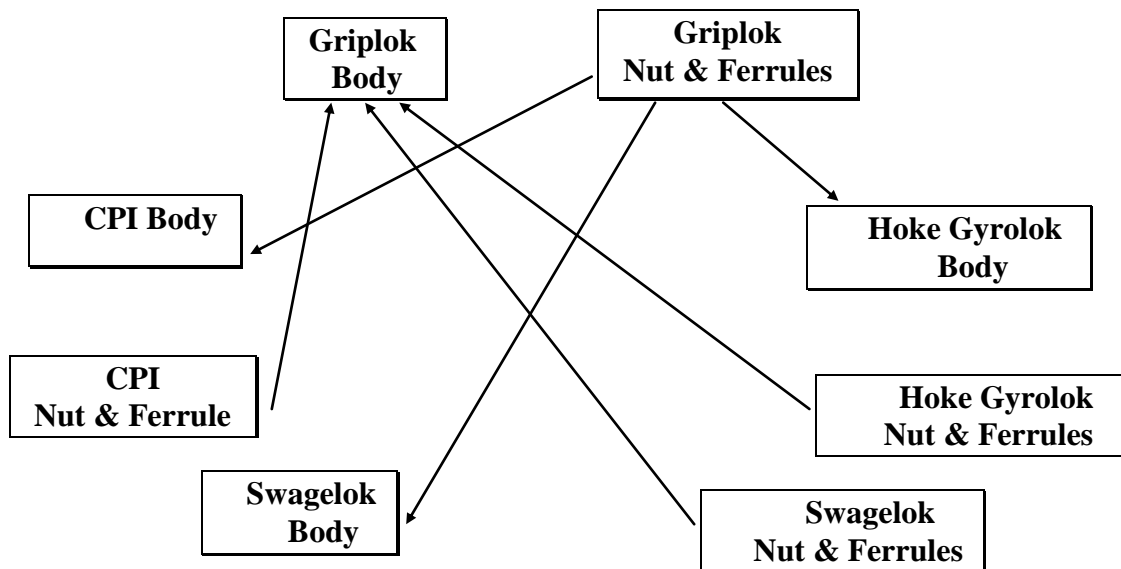


Figure 3.8.1, Interchange Test Combinations



Figure 3.8.2, Interchange Test Fittings and Components

Test Procedure: The tube fitting assembly is subjected to the Gas Leak Test (see Section 3.9), and then the Burst Test (see Section 3.2).

Acceptance Criteria: Gas Leak Test: The tube fitting assembly is to sustain an air booster test pressure, PSIG, of the ANSI / ASME maximum allowable working pressure of the tubing, up to a maximum pressure of 10,000 PSIG. Failure is any observed air leakage bubble.

Burst Test: The tube fitting assembly is to sustain a hydrostatic pressure, without observed leakage, exceeding a minimum of 4 times the ANSI / ASME maximum allowable working pressure of the tubing. Failure is to be by tubing burst, not by tube push out from fitting.

Test Results: Example results are shown in Table 3.8.0 below.

Results: Interchange Test

| Sample | Tubing / Fitting | | Acceptance Criteria | | | | Combinations | | Gas Leak Test | | Burst Test | | |
|--------|------------------|-------|---------------------|------------------|-----------------|-------------|-------------------|----------|---------------|-----------|--------------|-----------|-----------|
| | Size No. | Wall | W.P. | Burst = 4 X W.P. | Gas Leak Press. | Leak | Nut & Ferrule (s) | Body | Leak | Pass Fail | Actual Burst | Fail Type | Pass Fail |
| # | # | in | psig | psig | psig | Leak / None | name | name | Leak / None | P / F | psig | n/a | P / F |
| 1 | 8 | 0.035 | 2,450 | 9,800 | 2,450 | | Swagelok | Griplok | None | P | 12,260 | Tube | P |
| 2 | | | | | | | | | None | P | 12,260 | Tube | P |
| 3 | | | | | | | Gyrolok | Griplok | None | P | 10,430 | Tube | P |
| 4 | | | | | | | | | None | P | 10,430 | Tube | P |
| 5 | | | | | | | CPI | Griplok | None | P | 12,350 | Tube | P |
| 6 | | | | | | | | | None | P | 12,350 | Tube | P |
| 7 | | | | | | | Griplok | CPI | None | P | 12,370 | Tube | P |
| 8 | | | | | | | | | None | P | 12,370 | Tube | P |
| 9 | | | | | | | Griplok | Swagelok | None | P | 12,350 | Tube | P |
| 10 | | | | | | | | | None | P | 12,350 | Tube | P |
| 11 | | | | | | | Griplok | Gyrolok | None | P | 12,330 | Tube | P |
| 12 | | | | | | | | | None | P | 12,330 | Tube | P |
| 1 | 8 | 0.083 | 6,250 | 25,000 | 6,250 | | Swagelok | Griplok | None | P | 27,550 | Tube | P |
| 2 | | | | | | | | | None | P | 27,550 | Tube | P |
| 3 | | | | | | | Gyrolok | Griplok | None | P | 27,850 | Tube | P |
| 4 | | | | | | | | | None | P | 27,850 | Tube | P |
| 5 | | | | | | | CPI | Griplok | None | P | 27,600 | Tube | P |
| 6 | | | | | | | | | None | P | 27,600 | Tube | P |
| 7 | | | | | | | Griplok | CPI | None | P | 27,550 | Tube | P |
| 8 | | | | | | | | | None | P | 27,550 | Tube | P |
| 9 | | | | | | | Griplok | Swagelok | None | P | 27,530 | Tube | P |
| 10 | | | | | | | | | None | P | 27,530 | Tube | P |
| 11 | | | | | | | Griplok | Gyrolok | None | P | 27,640 | Tube | P |
| 12 | | | | | | | | | None | P | 27,640 | Tube | P |

Table 3.8.0 Example Interchange Test Results

Conclusions: All interchanged Griplok assemblies met or exceeded the approved Acceptance Criteria. All Griplok tube fittings sustained the required maximum allowable working pressure without leakage, and held leak free to tubing burst without exhibiting tube push out from the fitting.

Section 3.9: Gas Leak Test

Purpose: Test determines if the tube fitting assembly has adequate gas pressure-retaining capability, based on the ANSI / ASME B 31.3 maximum allowable working pressure of the tubing.

Equipment & Configuration: Two fittings are tested at a time – one on each end of a 4 ½” long test tube, per Initial Makeup Test (see Section 3). Samples of both minimum and maximum recommended wall tubing (worst case conditions) are used for each tested product configuration. See Figure 3.9.1 - 2, Gas Leak Test Configuration.

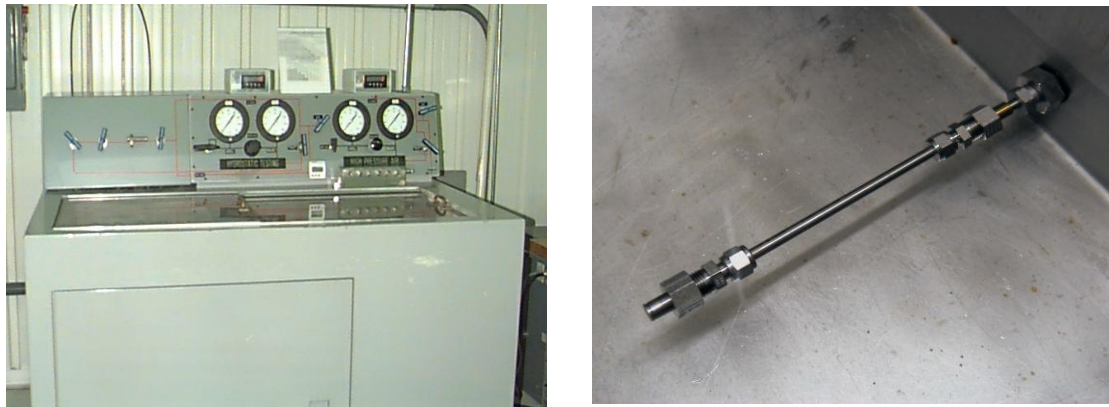


Figure 3.9.1 - 2, Gas Leak Test Configuration.

Test Procedure: The tube fitting assembly is pressurized, under water, with air in regular pressure increments to the lower of either the maximum allowable working pressure of the tubing or 10,000 PSIG, is attained. This pressure is held for a minimum of five minutes. The digitally displayed maximum pressure, in PSIG, is recorded

Acceptance Criteria: The tube fitting assembly is to sustain an air booster test pressure, PSIG, of the ANSI / ASME maximum allowable working pressure of the tubing, up to a maximum pressure of 10,000 PSIG. Failure is any observed air leakage bubble.

Test Results: Example results are shown in Table 3.9.0 below.

Results: Gas Leak Test

| Test | Sample No. | | Tubing / Fitting | | Acceptance Criteria | | | | Gas Leak | |
|-------------|------------|----|------------------|-------|---------------------|---------------------|----------------|----------------|----------------|--------------|
| | A | B | Size | Wall | W.P. | Burst = 4 x W.P. | Test Press. | Leak | A.C. Leak | Pass Fail |
| | # | # | # | in | psig | psig | psig | Leak / None | Leak / None | P / F |
| Gas Leak | 1 | 2 | 8 | 0.035 | 2,450 | 9,800 | 2,450 | None | None | P |
| | 3 | 4 | | | | | | | None | P |
| | 5 | 6 | | | | | | | None | P |
| | 7 | 8 | | | | | | | None | P |
| | 9 | 10 | | | | | | | None | P |
| | 11 | 12 | | | | | | | None | P |
| | 1 | 2 | | 0.083 | 6,250 | 25,000 | 6,250 | None | None | P |
| | 3 | 4 | | | | | | | None | P |
| | 5 | 6 | | | | | | | None | P |
| | 7 | 8 | | | | | | | None | P |
| | 9 | 10 | | | | | | | None | P |
| | 11 | 12 | | | | | | | None | P |

NOTE: A.C. = Acceptance Criteria

Table 3.9.0 Example Gas Leak Test Results

Conclusions: All Griplik assemblies met or exceeded the approved Acceptance Criteria. No Griplik tube fitting assemblies developed observable Gas Leakage.

Section 3.10: Thermal Cycle, Thermal Shock Test

Purpose: Test determines if the tube fitting assembly has the capability to sustain substantial and rapid temperature cycling while maintaining vacuum and pressure retention capabilities.

Equipment & Configuration: One fitting is tested at a time on the end of a test tube, assembled per Initial Makeup Test (see Section 3). Samples of both minimum and maximum recommended wall tubing (worst case conditions) are used for each tested product configuration. See Figure 3.10.1 - 2, Thermal Cycle, Thermal Shock Test Configuration.

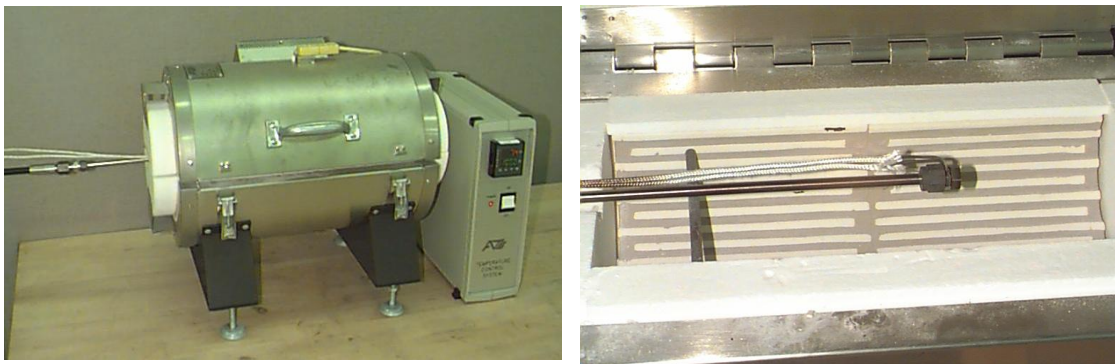


Figure 3.10.1 - 2, Thermal Cycle, Thermal Shock Test Configuration.

Test Procedure: A thermocouple is directly attached to the fitting to ensure accurate achievement of test temperature. The tube fitting assembly is pressurized with air to 1,000 PSIG, and simultaneously heated in a tubular furnace to 1,000 °F (538 °C). The digitally displayed maximum pressure, in PSIG, and temperature is recorded. On reaching both pressure and temperature the tube fitting assembly is removed and rapidly cooled to ambient temperature. This cycle is repeated three times.

The above thermal cycling is followed by a vacuum test whereby a high vacuum is drawn on the inside of the fitting by Vacuum Test Equipment, helium gas is sprayed over the outside of the fitting and a leakage rate is recorded.

Acceptance Criteria: The tube fitting assembly is to sustain the above thermal cycling under air pressure, and after quenching to room temperature not exhibit any detectable leakage when immersed in water. Additionally, when subsequently subjected to the vacuum test, the fitting must not exhibit a helium vacuum test leak rate in excess of $< 4 \times 10^{-9}$ mbar l/s.

Test Results: Example results are shown in Table 3.10.0 below.

Results: Thermal Cycle, Vacuum Tests

| Sample | Tubing | | Acceptance Criteria | | | Cycle No. | Vacuum Test | |
|--------|----------|---------------|---------------------|-------------|-----------|-----------|------------------|-----------|
| | Size No. | Wall | Temperature Range | Test Press. | Leak Rate | | Actual Leak Rate | Pass Fail |
| # | in | in | °F | psig | atm cc/s | # | atm cc/s | P / F |
| 1 | 8 | 0.035 | Amb. to 1,000 | 1,000 | 1.00E-08 | 1 | | |
| | | | | | | 2 | | |
| | | | | | | 3 | .3E-09 | P |
| 2 | | | | | | 1 | | |
| | | | | | | 2 | | |
| | | | | | | 3 | .2E-09 | P |
| 3 | | | | | | 1 | | |
| | | | | | | 2 | | |
| | | | | | | 3 | .1E-09 | P |
| 4 | | | | | | 1 | | |
| | | | | | | 2 | | |
| | | | | | | 3 | .7E-09 | P |
| 5 | | | | | | 1 | | |
| | | | | | | 2 | | |
| | | | | | | 3 | .1E-09 | P |
| 1 | 0.083 | Amb. to 1,000 | 1,000 | 1.00E-08 | 1 | | | |
| | | | | | 2 | | | |
| | | | | | 3 | .1E-09 | P | |
| 2 | | | | | 1 | | | |
| | | | | | 2 | | | |
| | | | | | 3 | .1E-09 | P | |
| 3 | | | | | 1 | | | |
| | | | | | 2 | | | |
| | | | | | 3 | 1.3E-09 | P | |
| 4 | | | | | 1 | | | |
| | | | | | 2 | | | |
| | | | | | 3 | .8E-08 | P | |
| 5 | | | | | 1 | | | |
| | | | | | 2 | | | |
| | | | | | 3 | .9E-08 | P | |

NOTE: A.C. = Acceptance Criteria

Table 3.10.0 Example Thermal Cycle Test Results

Conclusions: All Griplik assemblies met or exceeded the approved Acceptance Criteria. Observed leak rates of tested Griplik tube fitting assemblies performed consistently better than the required Acceptance Criteria, and published competitive results.

Section 3.11: Vacuum Test

Purpose: Test determines if the tube fitting assembly has the capability to seal at high vacuums, with ultra low leakage rates.

Equipment & Configuration: One fitting is tested at a time on the end of a piece of tubing, assembled per Initial Makeup Test (see Section 3). Samples of both minimum and maximum recommended wall tubing (worst case conditions) are used for each tested product configuration. See Figure 3.11.1 - 2, Vacuum Test Configuration.

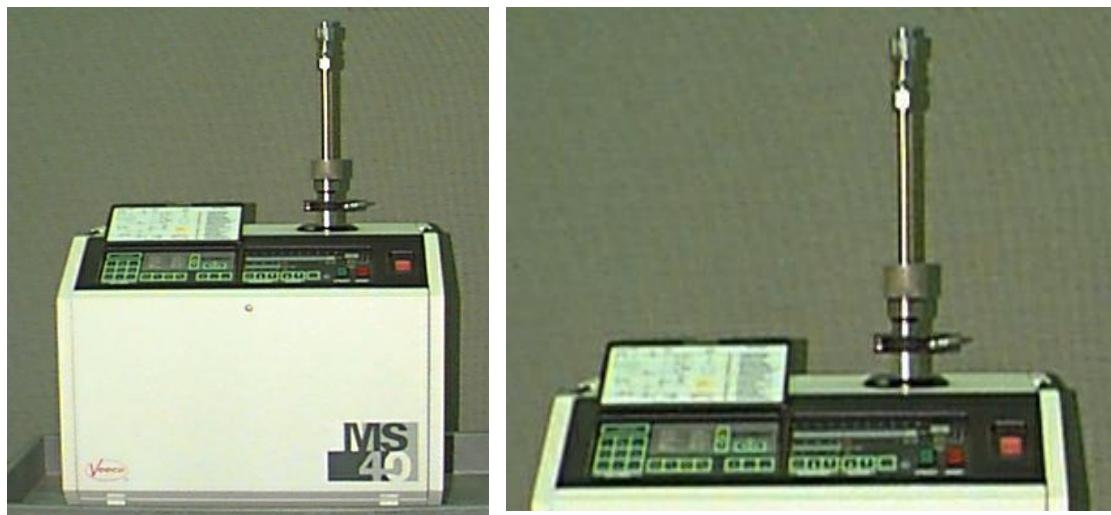


Figure 3.11.1 - 2, Vacuum Test Configuration


The Leak Rate Sensitivity of the Veeco MS-40 Helium Leak Detection Test Equipment is 4.0×10^{-11} mbar l/s. Griplik fittings have been tested and shown results in the 10^{-11} mbar l/s range.

Test Port pressure is displayed in units of milli-Torr. The vacuum levels developed during testing are as low as 4 mT - 9mT. This equates to an absolute pressure of .0000744 - 0.000174 PSIA.

Test Procedure: The internal volume of the tube fitting assembly is evacuated to a vacuum of 4 mT – 9 mT (milli-Torr). The digitally displayed vacuum pressure, in mT, is recorded. On achieving full vacuum pressure, helium gas is sprayed around the outside of the fitting, and the leakage rate is recorded.

Acceptance Criteria: The tube fitting assembly is to sustain the above vacuum pressure, and not exhibit a helium test leak rate in excess of $< 4 \times 10^{-9}$ mbar l/s.

What this ultra low level Leak Rate means in practical terms is shown in the following table, which gives the time (in months, years) it would take for the listed Leak Rates to fill one cubic inch of volume with air to atmospheric pressure at ambient temperature:



1 Cubic Inch

| <u>Fitting Leak Rate</u> | <u>Time for Fitting Leak to fill 1.0 in³ @ 1 Atmosphere Pressure</u> |
|--------------------------------|---|
| 1.0×10^{-6} mbar l/s | 6.3 months (192 days) |
| 1.0×10^{-9} mbar l/s | 527 years |
| 1.0×10^{-11} mbar l/s | 52,655 years |

Conclusions: All Griplik assemblies met or exceeded the approved Acceptance Criteria. Observed leak rates of tested Griplik tube fitting assemblies performed consistently better than the required Acceptance Criteria, and published competitive results.

Section 3.12: Low Temperature (Cryogenic) Helium Leak Test

Purpose: Test determines if the tube fitting assembly has the capability to seal in low temperature (cryogenic) applications with ultra low leakage rates.

Equipment & Configuration: One fitting is tested at a time on the end of a test tube, assembled per Initial Makeup Test (see Section 3). Samples of tubing with the minimum recommended wall thickness (worst case condition) are used for each tested product configuration. See Figure 3.12.1, Low Temperature Helium Leak Test Configuration.



Figure 3.12.1, Low Temperature Helium Leak Test Configuration.

The Leak Rate Sensitivity of the Veeco MS-40 40 Helium Leak Detection Test Equipment is 4.0×10^{-11} std cc/sec. Griplok tube fittings have been tested and shown results in the 10^{-11} mbar l/s range.

Test Port pressure is displayed in units of milli-Torr. The vacuum levels developed during testing are as low as 4 mT - 9mT. This equates to an absolute pressure of .0000744 - 0.000174 PSIA.

Test Procedure: The tube fitting assembly is immersed in a liquid nitrogen bath, -320 °F (-196 °C), and the internal volume of the tube fitting assembly is evacuated to a vacuum of 4 mT – 9 mT (milli-Torr). The digitally displayed Low Temperature Helium Leak pressure, in mT, is recorded. Helium is also cooled to the liquid nitrogen temperature before being sprayed on the cold fitting exterior. On achieving full Low Temperature Helium Leak pressure, -320 °F (-196 °C) helium gas is sprayed around the outside of the fitting, and the leakage rate is recorded.


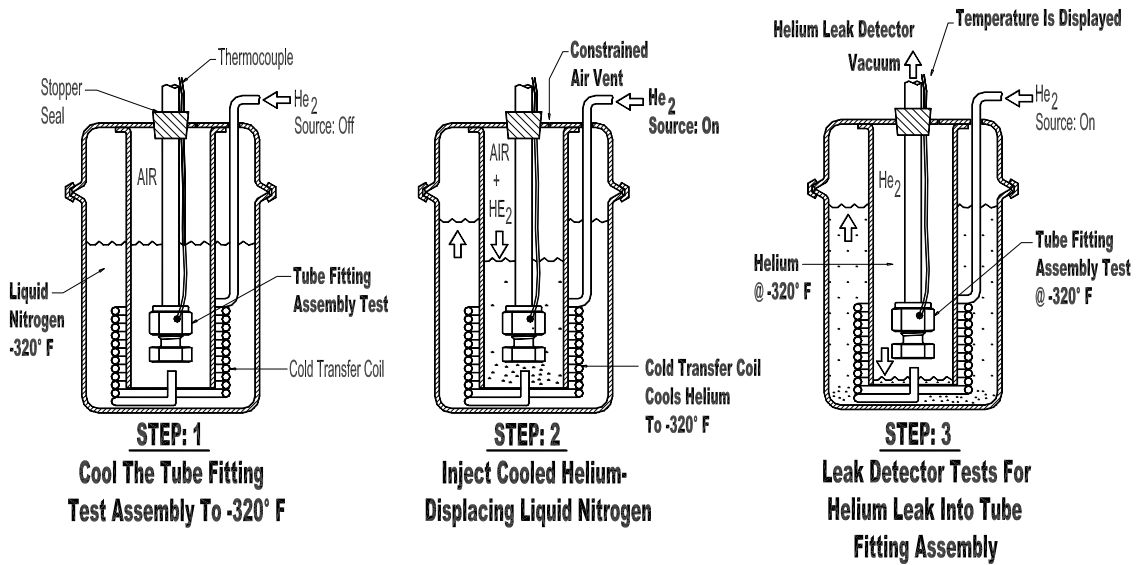


Figure 3.12.2, Low Temperature Helium Leak Test Sequence.

Acceptance Criteria: The tube fitting assembly is to sustain the above low temperature, and not exhibit a helium test leak rate in excess of $< 4 \times 10^{-9}$ mbar l/s.

What this ultra low level Leak Rate means in practical terms is shown in the following table, which gives the time (in months, years) it would for the listed Leak Rates to fill one cubic inch of volume with air to atmospheric pressure at ambient temperature:

1 Cubic Inch



Fitting Leak Rate

1.0×10^{-6} mbar l/s
 1.0×10^{-9} mbar l/s
 1.0×10^{-11} mbar l/s

Time for Fitting Leak to fill 1.0 in³ @ 1 Atmosphere Pressure

6.3 months (192 days)
 527 years
 52,655 years

Conclusions: All Griplik assemblies met or exceeded the approved Acceptance Criteria. Observed leak rates of tested Griplik tube fitting assemblies performed consistently better than the required Acceptance Criteria, and published competitive results.

Section 14: Bibliography, Equipment, References

Table 4.1: ASTM Material Standards

| Standard | Material Shape | Description |
|----------|------------------------|--|
| A 182 | Forged Fittings, Parts | Standard Specification for Forged or Rolled Alloy-Steel Pipe Flanges, Forged Fittings, and Valves and Parts for High-Temperature Service |
| A 276 | Bars | Standard Specification for Stainless Steel Bars and Shapes |
| A 479 | Bar, Shapes | Standard Specification for Stainless Steel Bars and Shapes for Use in Boilers and Other Pressure Vessels |
| B 16 | Bar, Shapes | Standard Specification for Free-Cutting Brass Rod, Bar and Shapes for Use in Screw Machines |
| B 124 | Bar, Shapes | Standard Specification for Copper and Copper Alloy Forging Rod, Bar, and Shapes |
| B 453 | Bar, Shapes | Standard Specification for Copper-Zinc-Lead Alloy (Leaded-Brass) Rod |
| A 179 | Tube | Standard Specification for Seamless Cold-Drawn Low-Carbon Steel Heat-Exchanger and Condenser Tubes |
| A 213 | Tube | Standard Specification for Seamless Ferritic and Austenitic Alloy-Steel Boiler, Superheater, and Heat-Exchanger Tubes |
| A 249 | Tube | Standard Specification for Welded Austenitic Steel Boiler, Superheater, Heat-Exchanger, and Condenser Tubes |
| A 269 | Tubing | Standard Specification for Seamless and Welded Austenitic Stainless Steel Tubing for General Service |
| B 68 | Tube | Standard Specification for Copper Tube, Bright Annealed |
| B 75 | Tube | Standard Specification for Seamless Copper Tube |
| B 88 | Tube | Standard Specification for Seamless Copper Water Tube |

Table 4.2: Applicable Codes and Standards

| Section | Test Description |
|------------------------------|---|
| ANSI / ASME B 31.1 | Power Piping Code |
| ANSI / ASME B 31.3 | Process Piping Code |
| ANSI / ASME BPV Section VIII | Boiler & Pressure Vessel Code |
| ISO 7257 | Aircraft - Hydraulic tubing joints and fittings - Rotary flexure test |

Table 4.3: Validation Test Equipment

| Section | Test Description | Test Equipment Description |
|---------|---|--|
| 3.1 | Initial Makeup Test..... | 1016702 Torque Wrench |
| 3.2 | Hydrostatic Burst Pressure Test..... | 1279 Ashcroft Pressure Gage L-400 Maximator Liquid Pump |
| 3.3 | Hydraulic Impulse Pressure Test..... | PDCR 911 Druck Pressure Transducer 451279 SSL 02B Ashcroft Pressure Gage |
| 3.4 | Repeated Remake Test..... | DLE 15-75 Maximator Air Booster Pump L-400 Maximator Liquid Pump |
| 3.5 | Tension Force Test..... | FI-90 Force Indicator 31910 Load Cell DTM Dillon Tensile Tester |
| 3.6 | Vibration Stress / Endurance Test..... | 42-05000W160S SC Hydraulic Engineering Booster Pump 2100 Strain Gage Conditioner System. The Measurements Group |
| 3.7 | Intermix Assurance Test..... | DLE 15-75 Maximator Air Booster Pump L-400 Maximator Liquid Pump |
| 3.8 | Interchange Assurance Test..... | DLE 15-75 Maximator Air Booster Pump L-400 Maximator Liquid Pump |
| 3.9 | Gas Pressure Leak Test..... | HP 224 McDaniels Pressure Gage DLE 15-75 Maximator Air Booster Pump |
| 3.10 | Thermal Cycle, Thermal Shock Test..... | 3210 Applied Test Systems Split Furnace XT16 Athena Temperature Controller MS-40 Veeco Helium Leak Detector |
| 3.11 | Vacuum Test..... | MS-40 Veeco Helium Leak Detector |
| 3.12 | Low Temperature (Cryogenic) Helium Leak Test..... | MS-40 Veeco Helium Leak Detector Type K TC Thermocouple |

TRADEMARKS:

Griplok is a trademark of SSP Fittings Corp.
A-Lok and CPI are trademarks of Parker Hannifin Corporation
Swagelok is a trademark of Swagelok Co.
Gyrolok is a trademark of Hoke Incorporated

SSP Instrumentation Document Number: ILGTR/000-02